

Features

Supports the SensL ArrayC-30035-144P-PCB
12x12 array of 3mm SiPMs

Horizontal signal connectors located on the back,
array located on the front

4-side tileable installation

Hybrid multiplexed readout

Four encoded position signals
for event centroid calculations: X+, X-, Y+, Y-

12 row signals and 12 column signals

DC-coupled signal path

Low power consumption

Patented diode-coupled charge division readout,
superior to traditional resistive readout

Improved spatial uniformity

Faster rise time

Reduced image noise


Precision temperature sensor

Four mounting holes for #2 hardware




SiPM array
not included

Front view

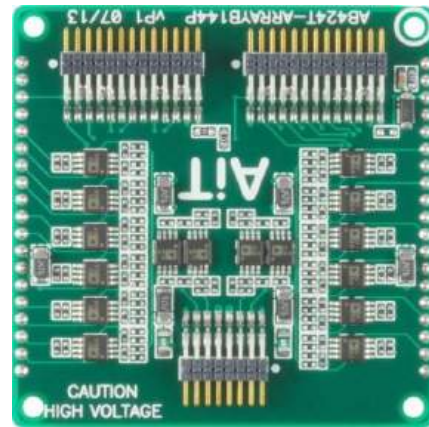

Back view

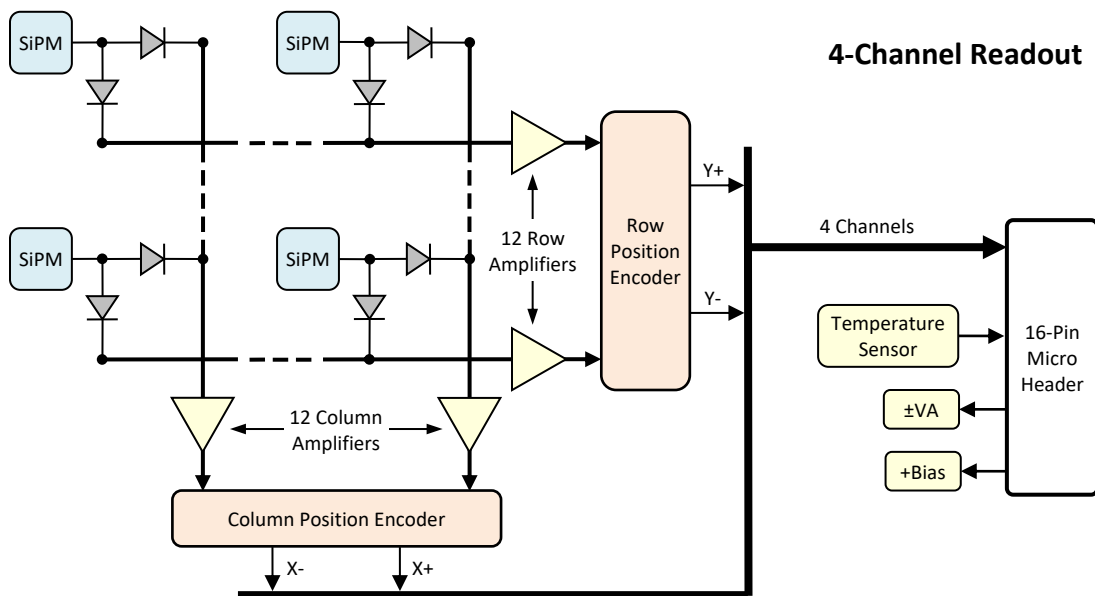


4-Channel Readout Specifications


Position Signal Outputs

Samtec FFSD-08-D-XX.XX-01-N
(XX.XX = length in inches)

Channel Map

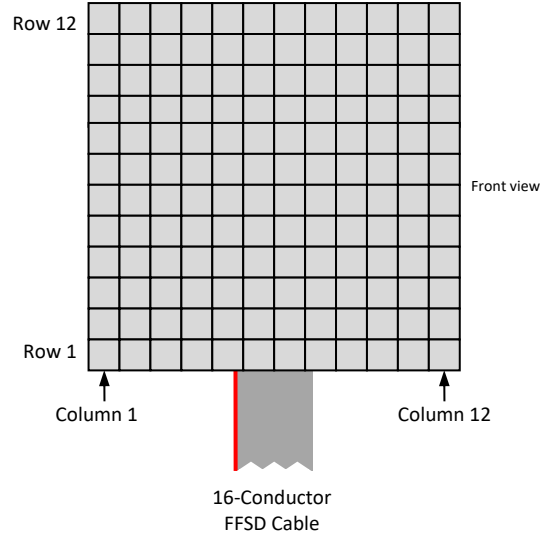

Signal Connector

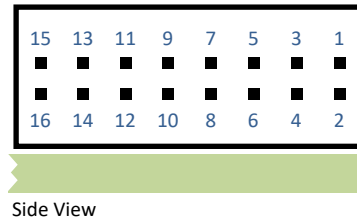

Pin	Function	Pin	Function
1	Temperature	2	Ground
3	X-	4	Ground
5	X+	6	Ground
7	-VA	8	Ground
9	+VA	10	Ground
11	Y-	12	Ground
13	Y+	14	Ground
15	+Bias	16	Ground

Row and Column Encoder Weights

Row# or Col# (for X- or Y-)	Row# or Col# (for X+ or Y+)	Fraction (ideal)	Fraction (actual)	% Error	Notes
1	12	0.0833	0.0833	0.00 %	Sum of X- and X+ fractions or Y- and Y+ fractions = 1.0833 Independent of signal position
2	11	0.1667	0.1650	-1.02 %	
3	10	0.2500	0.2483	-0.68 %	
4	9	0.3333	0.3311	-0.66 %	
5	8	0.4167	0.4167	0.00 %	
6	7	0.5000	0.5000	0.00 %	
7	6	0.5833	0.5882	0.84 %	
8	5	0.6667	0.6637	-0.45 %	
9	4	0.7500	0.7500	0.00 %	
10	3	0.8333	0.8333	0.00 %	
11	2	0.9167	0.9091	-0.83 %	
12	1	1.0000	1.0000	0.00 %	

Note: Errors exclude component tolerances

Output Signals

$$X- = (\text{SiPM signal}) * (\text{encoder gain}) * (X- \text{ fraction})$$

$$X+ = (\text{SiPM signal}) * (\text{encoder gain}) * (X+ \text{ fraction})$$

$$Y- = (\text{SiPM signal}) * (\text{encoder gain}) * (Y- \text{ fraction})$$

$$Y+ = (\text{SiPM signal}) * (\text{encoder gain}) * (Y+ \text{ fraction})$$

Typical event position calculation:

$$\mathbf{X \ column} = (X+ - X-) / (X+ + X-)$$

$$\mathbf{Y \ row} = (Y+ - Y-) / (Y+ + Y-)$$

Example

SiPM signal at column 4, row 3 (excluding encoder gain)

$$X- = (\text{Column 4 signal}) * 0.3311$$

$$X+ = (\text{Column 4 signal}) * 0.7500$$

$$Y- = (\text{Row 3 signal}) * 0.2483$$

$$Y+ = (\text{Row 3 signal}) * 0.8333$$

Row and Column Readout Specifications

Position Signal Outputs

Encoding	Charge division multiplexed to 12 rows and 12 columns
Gain	750Ω transimpedance gain
Output voltage	0 → -1V into 100Ω
Output impedance	100Ω
Output current	50mA maximum

Temperature Sensor

Output voltage	500mV + 10mV per °C
Output current	10mA
Output impedance	100Ω
Accuracy	±0.5°C

Bias Voltage



	+29V typical (refer to SiPM data)
Voltage clamp	47V Zener diode 500mW maximum

Amplifier Voltage (±VA)

	±2.8V → ±5.5V DC maximum
Current	±50mA typical at ±5.0V (I _q , no signal, no load)

Samtec FFSD-13-D-XX.XX-01-N
(XX.XX = length in inches)


Channel Map

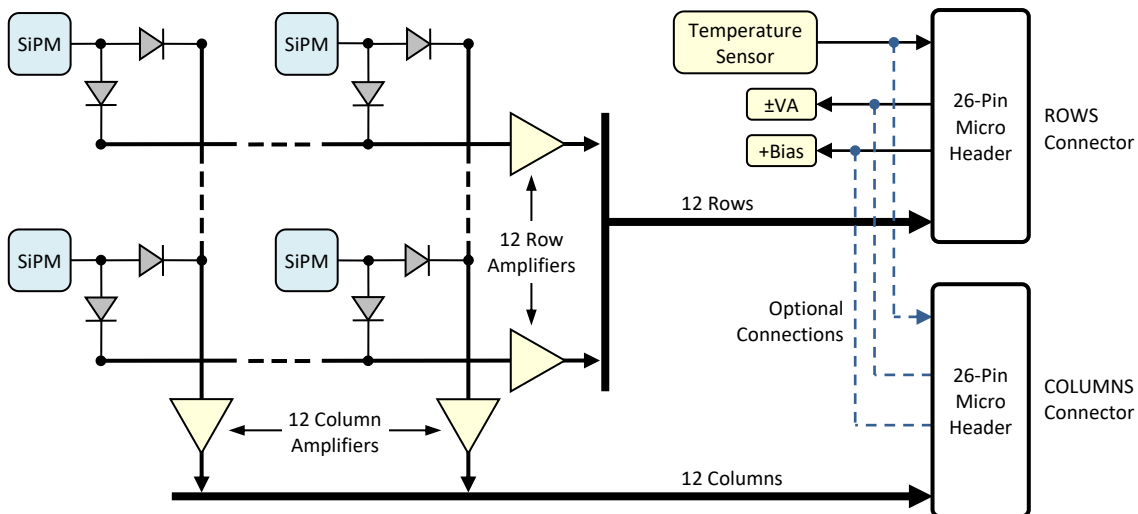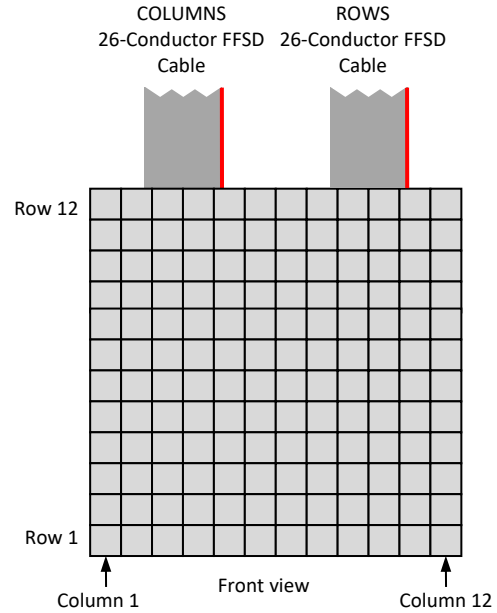

Row and Column Signal Connectors

ROWS

26-pin 0.050" horizontal header

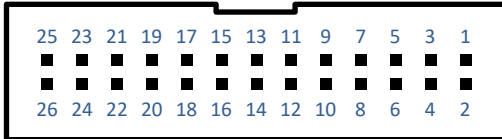


Side View

Pin	Function	Pin	Function
1	Row 1	2	Temperature
3	Row 2	4	Ground
5	Row 3	6	Ground
7	Row 4	8	Ground
9	Row 5	10	Ground
11	Row 6	12	-VA
13	Row 7	14	Ground
15	Row 8	16	+VA
17	Row 9	18	Ground
19	Row 10	20	Ground
21	Row 11	22	Ground
23	Row 12	24	Ground
25	+Bias	26	Ground

COLUMNS

26-pin 0.050" horizontal header

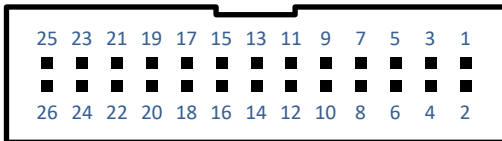

Side View

Pin	Function	Pin	Function
1	Column 1	2	Temperature
3	Column 2	4	Ground
5	Column 3	6	Ground
7	Column 4	8	Ground
9	Column 5	10	Ground
11	Column 6	12	*NC (-VA)
13	Column 7	14	Ground
15	Column 8	16	*NC (+VA)
17	Column 9	18	Ground
19	Column 10	20	Ground
21	Column 11	22	Ground
23	Column 12	24	Ground
25	*NC (+Bias)	26	Ground


NOTE

+Bias, +VA, -VA are normally connected to the ROWS connector. These signals are not connected to the COLUMNS connector. Disconnected signals are indicated as "NC". These signals can be optionally connected to the COLUMNS connector as an assembly variant.


Typical Signals

4-Channel Readout

Source = Laser; Receiver = ABR4, channel 1, minimum gain; Bias = +29V; FFSD cable = 36"

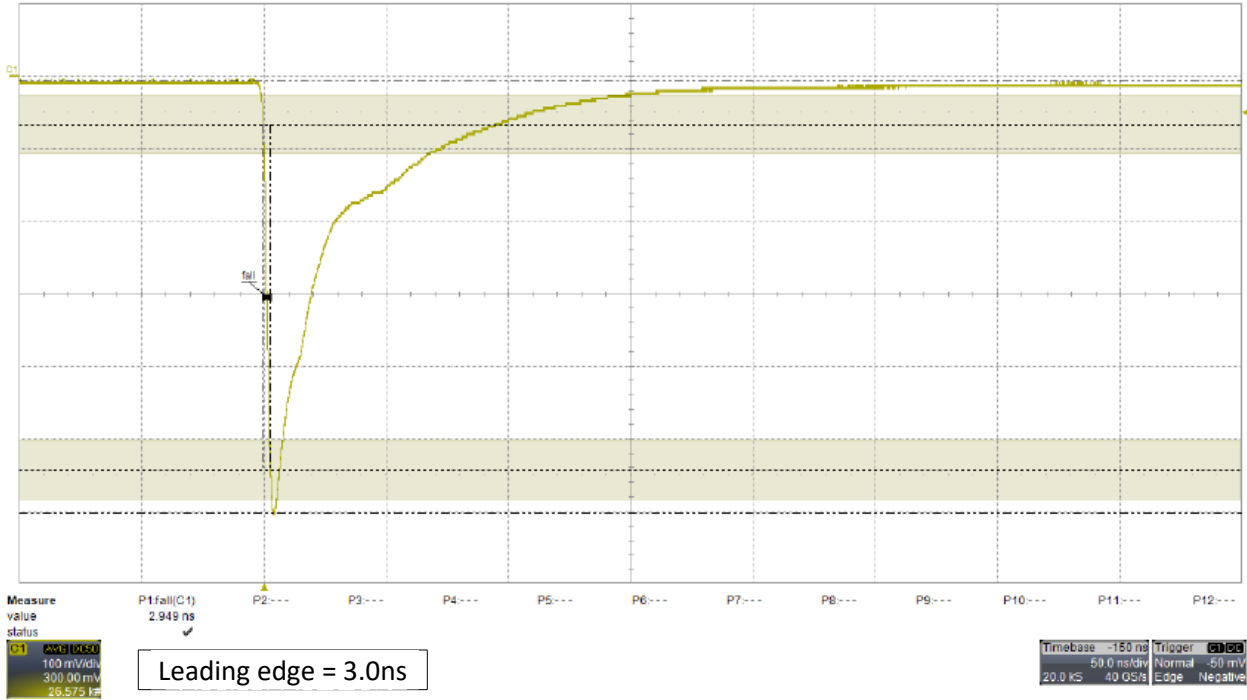


Source = LYSO emission; Receiver = ABR4, channel 1, minimum gain; Bias = +29.5V; FFSD cable = 36"; persistence display

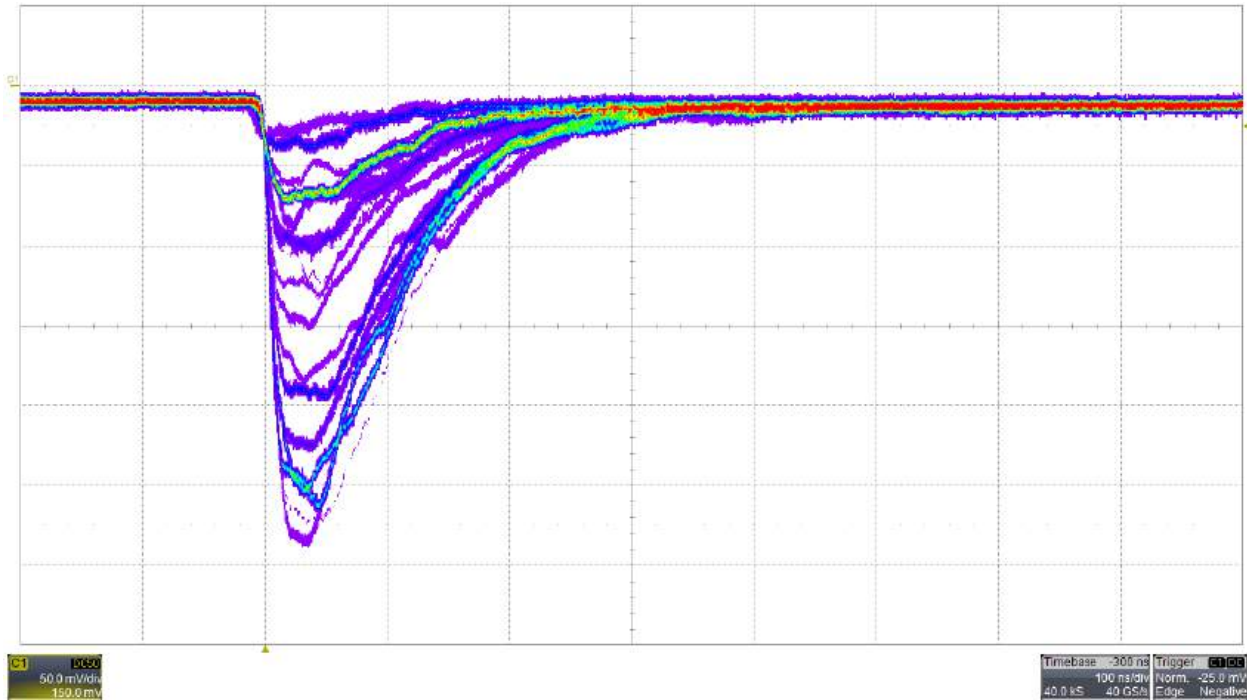


Mechanical

Front View

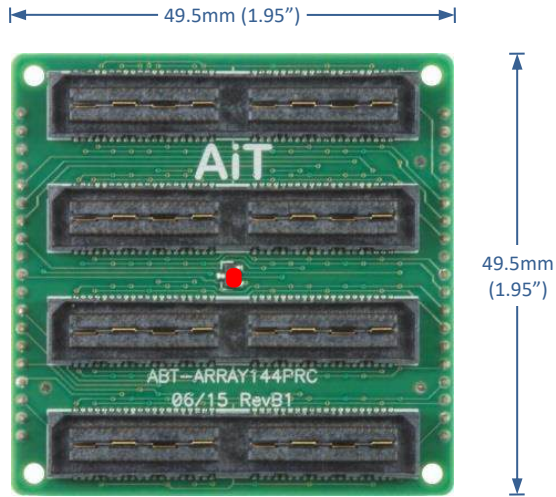


Back View

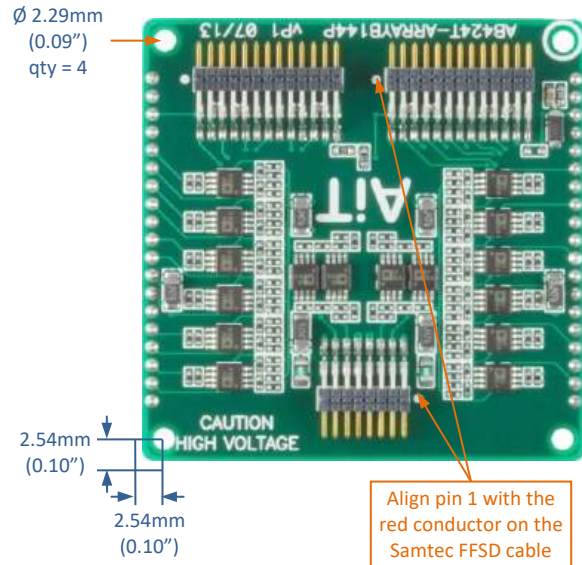


● Temperature sensor
Measurement tolerance: ±0.020"


Side View, Base Attached to Array

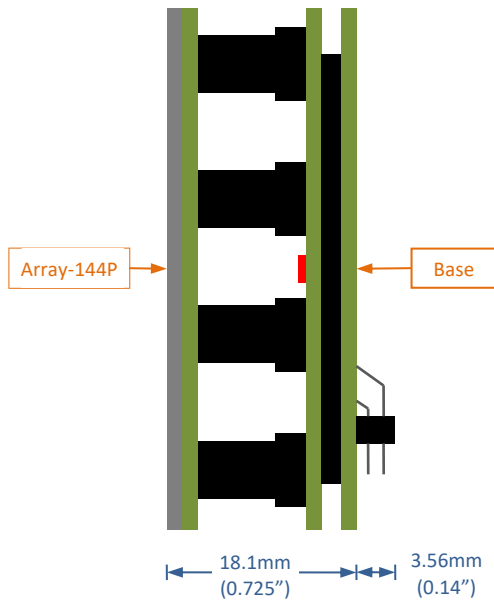

Side View, Base Only

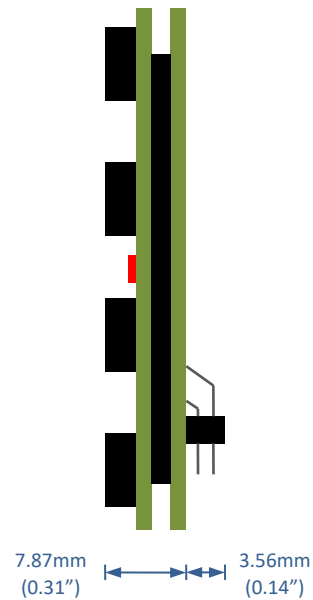

4-Channel Active Base Readout Kit

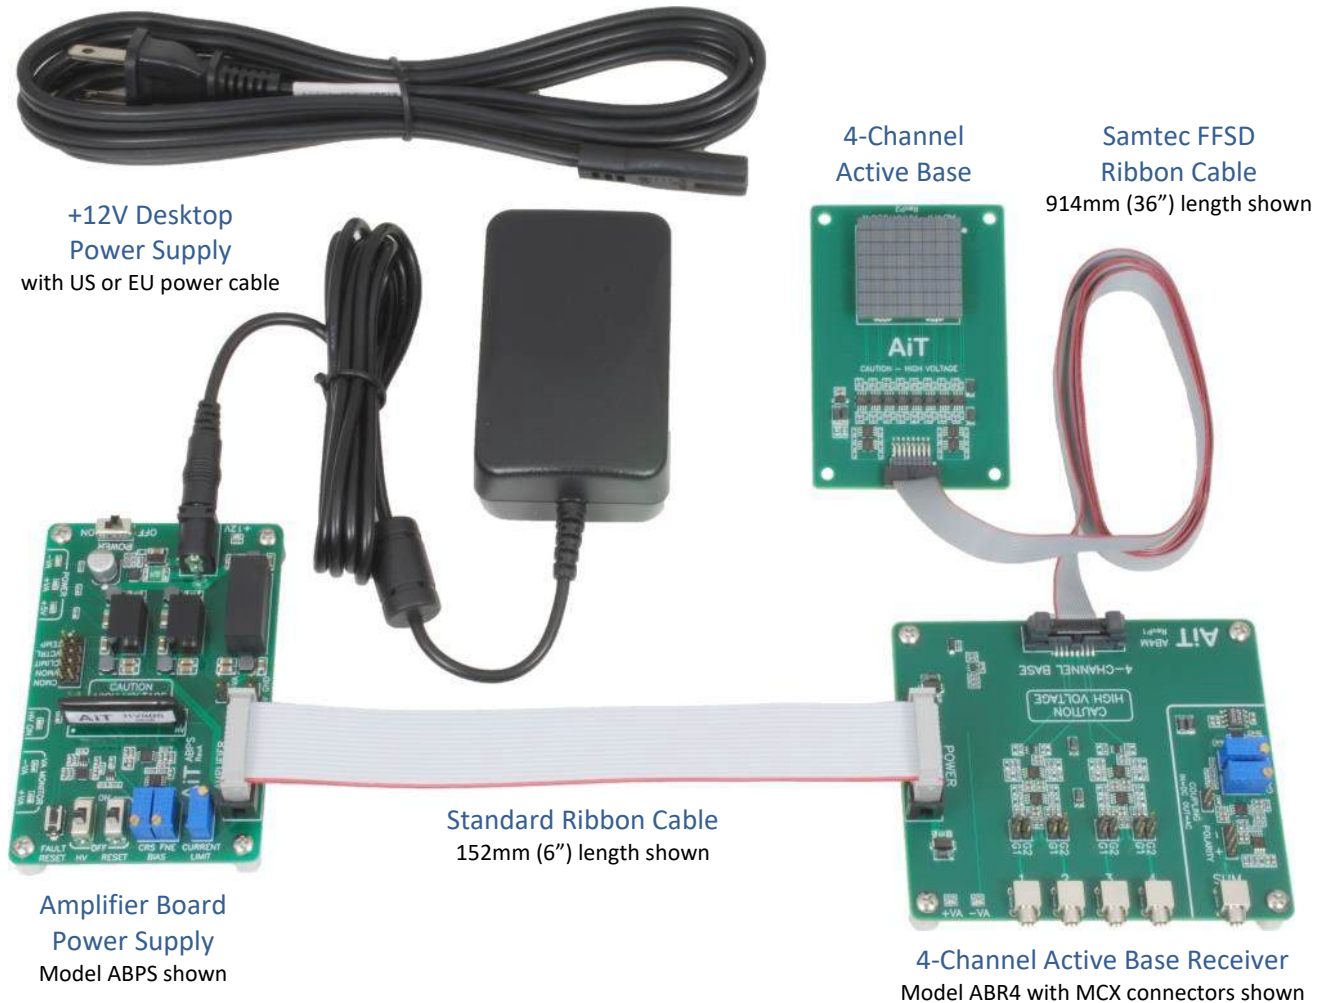

Components

Each component is available separately. Refer to each datasheet for details.

The Active Base includes a 914mm (36") Samtec FFSD micro-pitch ribbon cable.

The Amplifier Board Power Supply includes a 12V desktop power supply and a HV80 bias voltage power supply.

The 4-channel Active Base Receiver includes a 152mm (6") power supply ribbon cable and a breakout board to connect any external power supply.

Safety Information



WARNING – High Voltage

High voltage may be present during operation
High voltage stored on capacitors may be present after power is removed
Improper handling may result in personnel injury or equipment damage

This high-voltage device must be used only by personnel trained and qualified in safe handling, installation, and operation of high-voltage equipment.



CAUTION – Electrostatic Discharge (ESD) Sensitivity

The circuit board can be damaged by electrostatic discharge. Observe precautions for handling electrostatic sensitive devices. Handle only at static-safe workstations.

High-Gain Photodetectors

High-gain photodetectors such as silicon photomultipliers may conduct damaging currents if exposed to high optical signal levels while the bias voltage is applied, or if the bias voltage exceeds the recommended operating range. These devices must be operated only in low-light conditions, and only within the manufacturer's recommended bias voltage range.

Handling and Disassembly

This product may be provided with a protective enclosure. Disassembled enclosure components and circuit boards may contain sharp edges. Take appropriate safety precautions while assembling or disassembling the enclosure and handling disassembled components.

Indoor Use Only

Do not operate this product in a wet or damp environment. Do not operate in an explosive atmosphere.

Use of this product, and AiT Instruments' liability related to use of this product, is further governed by AiT Instruments' standard terms and conditions of sale, which were provided upon purchase of this product.